

LOC I-ILN 110.7	APP CRS 224°	Rwy Idg TDZE Apt Elev	10701 1077 1077
---------------------------	------------------------	-----------------------------	--

ILS or LOC RWY 22R

WILMINGTON AIR PARK (ILN)


DME or RADAR required for procedure entry.
ADF or DME required for LOC only.

Simultaneous approach authorized. DME from MXQ VOR/DME.
DME use requires simultaneous reception of I-ILN and MXQ DME.

ALSIF-2

MISSED APPROACH: Climb to 1600 then climbing right turn to 3500 on MXQ VOR/DME R-250 to KLARC INT/MXQ 10 DME/ RADAR and hold, continue climb-in-hold to 3500.

D-ATIS 124.925	COLUMBUS APP CON 118.85 269.275	WILMINGTON TOWER 119.475	GND CON 121.6	CLNC DEL 128.85
--------------------------	---	------------------------------------	-------------------------	---------------------------

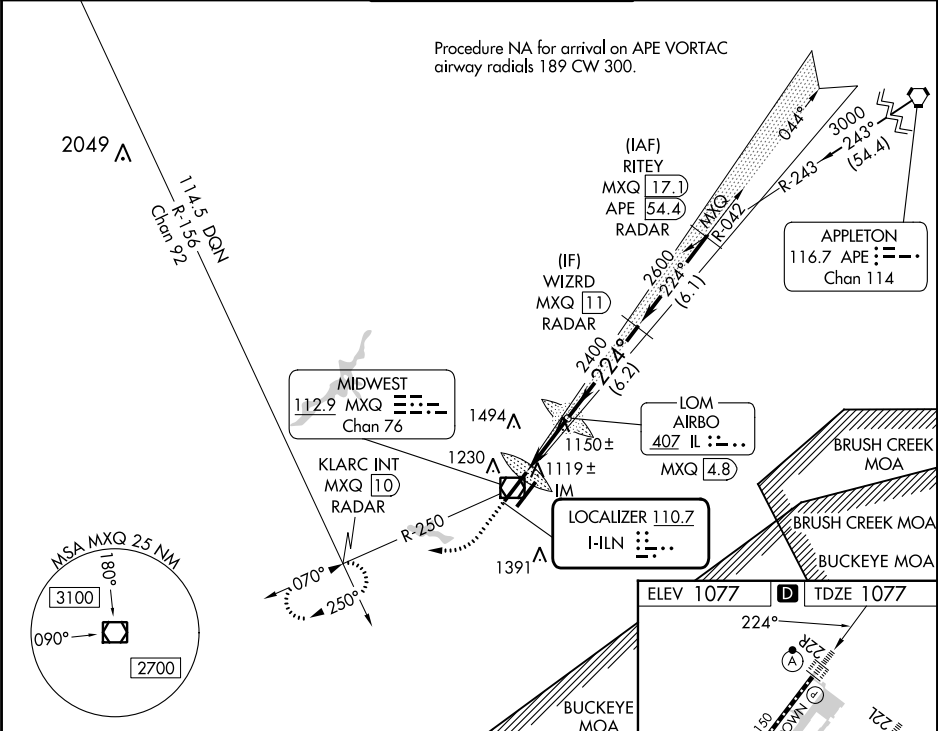

1600	3500	VGSI and ILS glidepath not coincident (VGSI Angle 3.00/TCH 71).			WIZRD MXQ 11 RADAR
		KLARC INT	AIRBO LOM MXQ 4.8		
CATEGORY	A	B	C	D	
S-ILS 22R	1277/18		200 (200-½)		
S-LOC 22R	1400/24	323 (400-½)	1400/26	323 (400-½)	
CIRCLING	1560-1	483 (500-1)	1860-2¼ 783 (800-2¼)	1860-2½ 783 (800-2½)	

